


Rapid Flexible tip Digital Thermometer

Model: DT-K111D

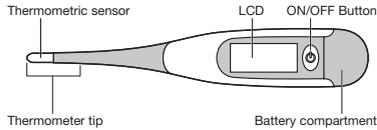

Congratulations on your purchase of this product. Please read the instructions carefully before using the thermometer for the first time, and keep these in a safe place. This product is intended for the measurement of human body temperature. This product is for home and hospital use, operator shall be at least 11 years old and patient can be operator.

Operating Instructions

Before using, please disinfect the probe at first. To switch on, press the ON/OFF button next to the display; a short beep will sound, indicating that the thermometer is operational. At the same time the thermometer runs a self-check test, during which all the digital segments appear on the LCD. When the letters "L" and a flashing "°C" or "°F" display, the thermometer is now ready for use. If the ambient temperature is below 32°C or 89.6°F, then "L°C" or "L°F" will appear on the LCD and if it is more than 42°C or 107.6°F, then "H°C" or "H°F" will appear on the LCD.

During the reading, the current temperature is displayed continuously and the "°C" or "°F" symbol flashes. The measurement is completed when a constant temperature value has been reached. The temperature value is considered constant when the temperature rises less than 0.1°C within 4 seconds. As soon as the constant temperature value is reached, a beep will sound 12 times, and the "°C" or "°F" symbol will stop flashing. The highest temperature measured appears on the LCD. However, please note that this thermometer is a maximum thermometer, i.e. the displayed temperature can increase slightly if measurement continues after the beep, this is particularly the case with axillary measurements, the temperature value should be recorded which approximates the core body temperature. In this instance please note the description under "Methods of measuring temperature". When the measurement is completed, please switch the thermometer off by pressing the ON/OFF button. After the temperature has been displayed, the thermometer will shut off automatically after 4 minutes and a beep sound.

Memory function

Switch the thermometer on, a short beep will sound. At the same time the thermometer runs a self-check test, during which all the digital segments appear on the LCD. After that the last reading value with "°C" or "°F" will appear automatically on the LCD for about 2 seconds. The reading is only over-written when a new temperature value is recorded.

Methods of measuring temperature

It is important to remember that the body temperature reading depends on the site where it is measured. For this reason, the measurement site must always be specified in order to ensure that a correct temperature reading is recorded.

In the rectum(rectal)

This is the most accurate method from a medical point of view, because it comes closest to the core body temperature. Lubricating the thermometer tip with unguing agents before use. Do not use vaseline. The

APPROVED

By cmlam at 3:53 pm, Jul 26, 2021

thermometer tip is inserted carefully into the rectum for a maximum of 13 mm. The usual measuring time is approximately 10 seconds.

Under the arm(axillary)

Placing the thermometer in the armpit provides a measurement of surface temperature that can fluctuate by around 0.5°C to 1.5°C from rectal temperature readings in adults. The usual measuring time for this method is approximately 23 to 29 seconds. It should be noted that an exact reading won't be obtained if, for example, the armpit temperature is lower than normal (the armpit temperature has been cooled down). If in this case, we recommend extending the measuring time by around 5 minutes in order to obtain the most precise possible reading that corresponds as closely as possible to the core body temperature.

In the mouth(oral)

There are different heat zones in the mouth. As a general rule, the oral temperature is 0.3°C to 0.8°C lower than the rectal temperature. To ensure that reading is as accurate as possible, place the thermometer tip to the left or right of the root of the tongue. The thermometer tip must have constant contact with the tissue during the reading and be placed under the tongue in one of the two heat pockets at the back, keep the mouth closed during the reading and breathe evenly through the nose. Do not eat or drink anything before the measurement. The usual measuring time is approximately 25 seconds.

Note: We strongly recommend the rectal method as the most accurate method for identifying the basal temperature, and advise you to extend the measuring time by 1 Minutes after the beep.

How to change the measuring unit

Under the power off state, press the ON/OFF button for 2 seconds, the display will show "L" and the unit in use. Press the ON/OFF button to switch the unit, Then the thermometer will be operational after 3 seconds.

Cleaning and disinfection

The best way to clean the thermometer tip is by applying a disinfectant (e.g. 70% medical alcohol) with a damp cloth. It shall be disinfected before each use. The Waterproof thermometers can be immersed in liquid or lukewarm water for through cleaning and disinfection.

Safety precautions

- The incorrect methods of measuring temperature may lead to inaccurate measurement results.
- Do not allow the device to come into contact with hot water.
- Do not expose to high temperatures or direct sunlight.
- Do not drop the thermometer. It is neither shock-proof nor impact-resistant.
- Do not modify this device without the authorization of the manufacturer.
- Do not bend or open the device (except the battery compartment).
- Do not clean with thinners, petrol or benzenel. Only clean with water or disinfectant.
- Do not immerse the Waterproof thermometers under water 15cm for longer than 30 minutes.
- The thermometer contains small parts (battery, battery this reason, do not leave the thermometer unattended in the hands of children.
- Avoid bending the thermometer tip by more than 45 degrees.
- If the ambient temperature is over 35°C or 95°F, dip the thermometer tip in cold water for approx. 5 to 10 seconds prior to measuring the temperature.
- Persistent fever, in particular in children, has to be treated by a doctor, please get in touch with your doctor!
- Do not use near strong electromagnetic fields, i.e. keep it away from any radio systems and mobile phones.

Battery replacement

The battery is low voltage and needs to replace when the "E" battery symbol appears on the right of The LCD Remove the battery cover. Pull out the inner frame gently, then take out the battery with a toothpick or tweezers, replace the battery of the same type. The electrode of battery: the "+" sign up and "-" sign down.

We advise you to remove the batteries if the device is not going to be used for a longer period of time.

The backlight of different thermometers will have differences, it may be related to the battery power or the versions of thermometer, attribute normal phenomenon.

Product disposal

Please ensure environmental protection. Batteries do not belong in the domestic waste. Please hand them in at collection point or the municipal recycle material centre as special waste. The lithium battery or fuel cell may lead to excessive temperatures, fire or explosion.

This symbol on products and/or accompanying documents means that consumed electronic products must not be mixed with conventional domestic waste. Take these products to the corresponding collection points for correct treatment and recycling, where they will be accepted free of charge. For more information on the closest collection point, Please enquire with your local authorities.

Technical data

Type: maximum thermometer

Measurement range: (32.0-42.0)°C/(89.6-107.6)°F

Measurement accuracy:

+/- 0.1°C/0.2°F (35.5°C-42.0°C/95.9°F-107.6°F)

+/- 0.2°C/0.4°F (32.0°C-35.5°C/89.6°F-95.9°F)

Storage/transportation temperature:

(-25-55)°C, ≤95%RH

Ambient temperature during use: (5-35)°C, ≤80%RH

Min Scale: 0.1°C/0.1°F

Battery type:

Lithium battery, type CR 1632, 3V, service life minimum

100 hours under continuous operation.

Weight: Approx. 19g

Display: Illuminated display

Atmospheric pressure: 700-1060hPa

Explanation of symbols

or Battery is empty Type BF equipment

Manufactured by Manufacture date

Product disposal instructions for electronic devices

Read the instructions (actual symbol colours are white on a blue background)

IP22 Classification according to the degree of protection against ingress of water as detailed in IEC 60529

The battery in this product complies with the requirements stated in European Directives 2006/66/EEC

CE CE conformity marking

Stand by

L°C or L°F: temperature under 32°C or 89.6°F
H°C or H°F: temperature over 42°C or 107.6°F

Legal requirements and guidelines

This product complies with the European Directive for Medical Devices 93/42/EEC and carries the CE mark. The device also complies with the specifications of the European Standard EN 12470-3 Clinical thermometers - Part 3: Performance of compact electrical thermometers (non-predictive and predictive) with maximum device. The CE marking confirms that this is a medical device with a measuring function in the sense of the Medical Devices Act which has undergone a conformity assessment procedure. A Notified Body confirms that this product fulfils all the appropriate statutory regulations.

Calibration check

This thermometer is initially calibrated at the time of manufacture. If this thermometer is used according to the operation instruction, periodic re-adjustment is not required. The calibration check has to be carried out immediately, if there are indications that the product does not keep the defined error limits or the calibration properties could have been affected by an intervention or by any other means. Please also observe any national statutory regulations. The calibration check can be carried out by the competent authorities or by authorised service providers. A test instruction for calibration check can be provided to the relevant authorities and authorised services providers on request.

Support

Our manual should provide you with all the information you need to set up and use this product.

If you have a question, have a look at our Troubleshooting page!

For further assistance, why not contact our Customer Care team directly? We're here to help!

Our Customer Care team are available from 9am-5pm, Monday to Friday (excluding bank holidays).

We promise to respond to all queries and will ensure to resolve any issue you may be having.

You can reach us by...

Phone (UK):
+44 1483 937967

Post (UK):
Kinetik Medical Devices Limited
Unit 3, Perrywood Business Park, Honeycrock Lane, Salfords, Redhill. RH11 5DZ

Phone (NZ):
(09) 801 0627

Post (NZ):
Kinetik Wellbeing NZ
44 John Brian Drive, 0794 Redvale, Albany, Auckland, New Zealand

Live Chat:
Simply visit www.kinetikwellbeing.com and send us a message.

Email:
customercare@kinetikwellbeing.com

Hangzhou Hua'an Medical & Health Instruments Co., Ltd
Building 2, 1# Fuzhuo Nan Rd, Wuchang Town,
Yuhang District, Hangzhou, Zhejiang 310023 China

Shanghai International Holding Corp. GmbH (Europe)
Elffestrasse 80, 20537 Hamburg Germany
E-Mail: shholding@otmail.com
Tel.: 049-40-2513175 Fax.: 049-40-255726

ELECTROMAGNETIC COMPATIBILITY INFORMATION

This device is suitable for home healthcare environment and professional healthcare facility environment.

WARNING: Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

The essential performance is the digital thermometer can offer the temperature measurement.

Do not use mobile (cellular) telephones and other devices, which generate strong electrical or electromagnetic fields, near the medical device. This may result in incorrect operation of the unit and create a potentially unsafe situation. Recommendation is to keep a minimum distance of 7 m. Verify correct operation of the device in case the distance is shorter.

Guidance and manufacturer's declaration – electromagnetic emissions		
The device is suitable for use in the specified electromagnetic environment and it has meets the following standard's emission requirements.		
Phenomenon	Profession healthcare facility environment	Home healthcare environment
Home healthcare environment	CISPR 11, Group 1, Class A or B	CISPR 11, Group 1, Class B
Harmonic distortion	IEC 61000-3-2, Class A or not applicable	NA
Voltage fluctuations and flicker	IEC 61000-3-3 or not applicable	NA

Guidance and manufacturer's declaration – electromagnetic immunity			
The device is suitable for use in the specified electromagnetic environment and it meets the following immunity test levels. Higher immunity levels may cause the device's essential performance lost or degraded.			
Phenomenon	Basic EMC standard or test method	Professional healthcare facility environment	Home healthcare facility environment
Electrostatic discharge	IEC 61000-4-2	+/- 8 kV contact +/- 2 kV, +/- 4 kV, +/- 8 kV, +/- 15 kV air	
Radiated RF EM fields	IEC 61000-4-3	3V/m 80MHz-2.7GHz 80%AM at 1kHz or 2Hz	10V/m 80MHz-2.7GHz 80%AM at 1kHz or 2Hz
		1kHz or 2Hz can be specified by the manufacturer	
Proximity fields from RF wireless communications equipment	IEC 61000-4-3	See the RF wireless communication equipment table in "Recommended minimum separation distances".	
Rated power frequency magnetic fields	IEC 61000-4-8	30A/m; 50 Hz or 60Hz	
Electric fast transients bursts	IEC 61000-4-4	NA	
	For input a.c. power port d.c. power lines or signal input/output lines whose length exceeding 3m		
Surges	IEC 61000-4-5	NA	
	For 1. input a.c. power port; 2. all d.c. power ports connected permanently to cables >3m 3. output signal output lines connected directly to outdoor cables		

Conducted disturbances induced by RF fields	IEC 61000-4-6	NA
	For 1. input a.c. power port; 2. all d.c. power ports connected permanently to cables >3m 3. all patient-coupled cables 4. SIP/SOP whose maximum cable length ≥ 3m	
Voltage dips	IEC 61000-4-11	NA
Voltage interruptions	IEC 61000-4-11	NA
UT: rated voltage(s); E.g. 25/30 cycles means 25 cycles at 50Hz or 30 cycles at 60Hz		

Recommended minimum separation distances						
Nowadays, many RF wireless equipments are being used in various healthcare locations where medical equipment and/or systems are used. When they are used in close proximity to medical equipment and/or systems, the medical equipment and/or systems' basic safety and essential performance may be affected. This device has been tested with the immunity test level in the below table and meet the related requirements of IEC 60601-1-2:2014. The customer and/or user should help keep a minimum distance between RF wireless communications equipment and this device as recommended below.						
Test frequency (MHz)	Band (MHz)	Service	Modulation	Maximum power(W)	Distance (m)	Immunity test level (V/m)
385	380-390	TETRA 400	Pulse modulation 18Hz	1.8	0.3	27
450	430-470	GMRS 460 FRS 460	FM ± 5 kHz deviation 1 kHz sine	2	0.3	28
710	704-787	LTE Band 13, 17	Pulse modulation 217Hz	0.2	0.3	9
745						
780						
810	800-960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation 18Hz	2	0.3	28
870						
930						
1720	1700-1990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3 4, 25; UMTS	Pulse modulation 217Hz	2	0.3	28
1845						
1970						
2450	2400-2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation 217Hz	2	0.3	28
5240	5100-5800	WLAN 802.11 a/n	Pulse modulation 217Hz	0.2	0.3	9
5500						
5785						