In association with


St John Ambulance

kinetik WELLBEING


- Quick Start Guide -

WT2


TENS
Pain Reliever
PennyPad

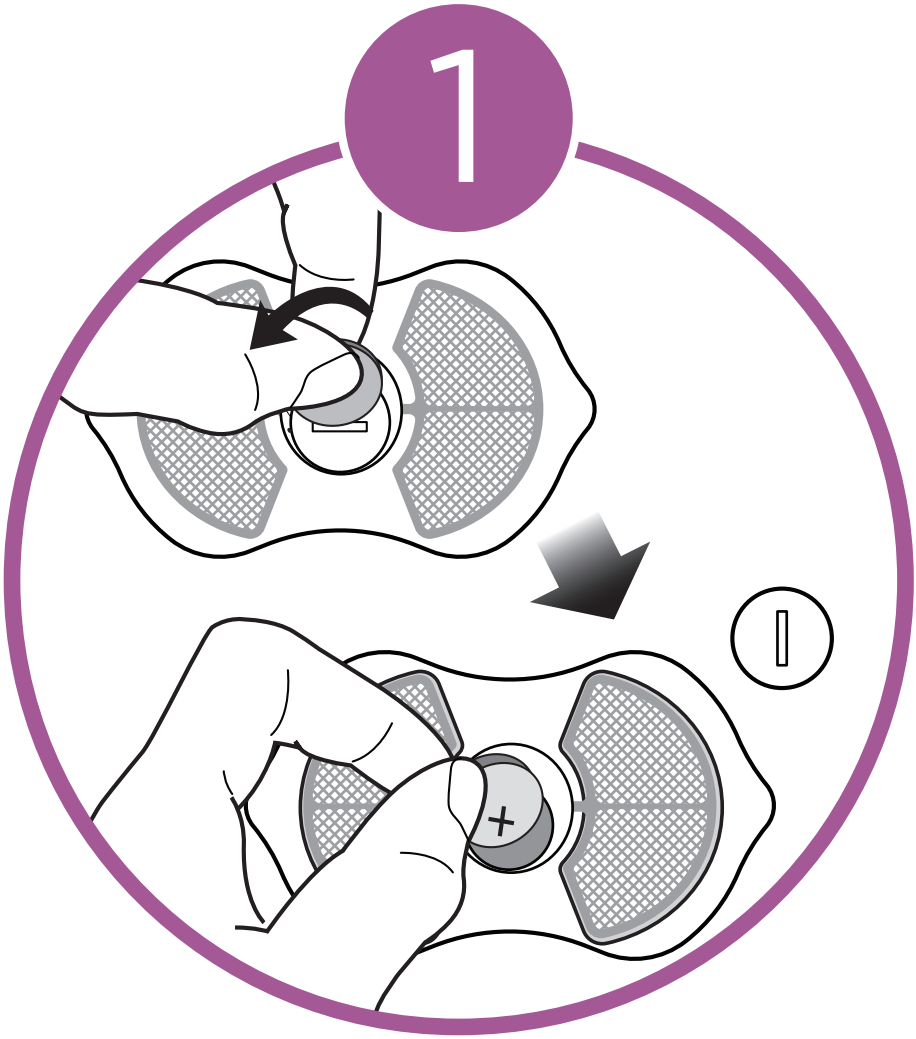

Ensure battery has been correctly inserted into device. Use coin tool provided to do so.

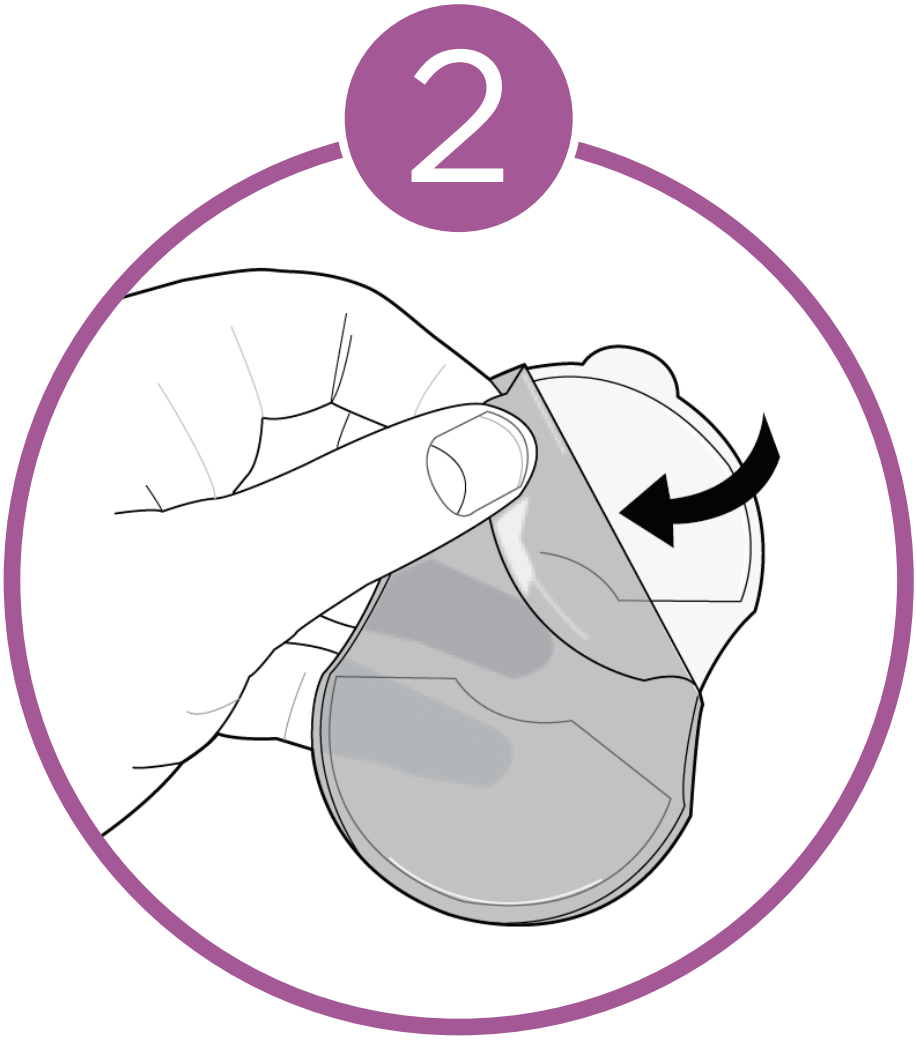


Remove
blue protective film
from gel pads.

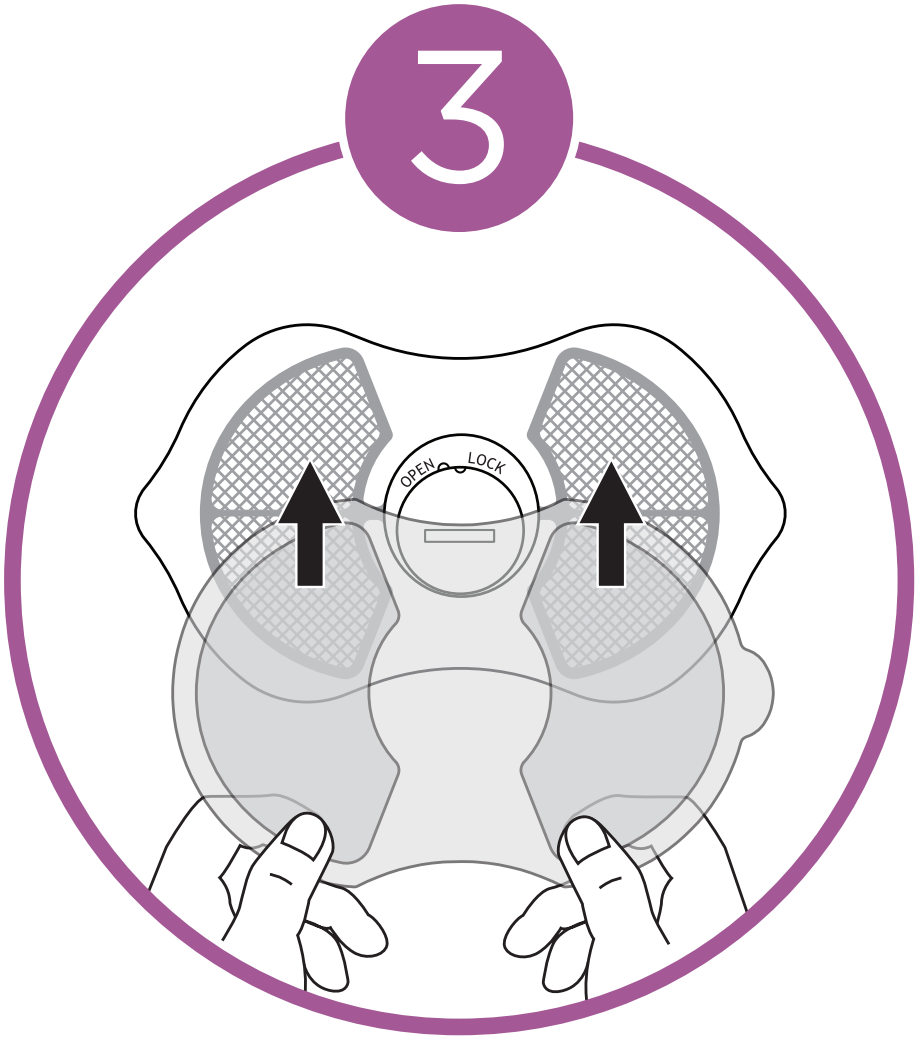


Place gel pads
over correct position
on back of device.
Ensure gel pads are
firmly secured.




Remove
clear protective film
from gel pads,
do not remove gel pads
from device.

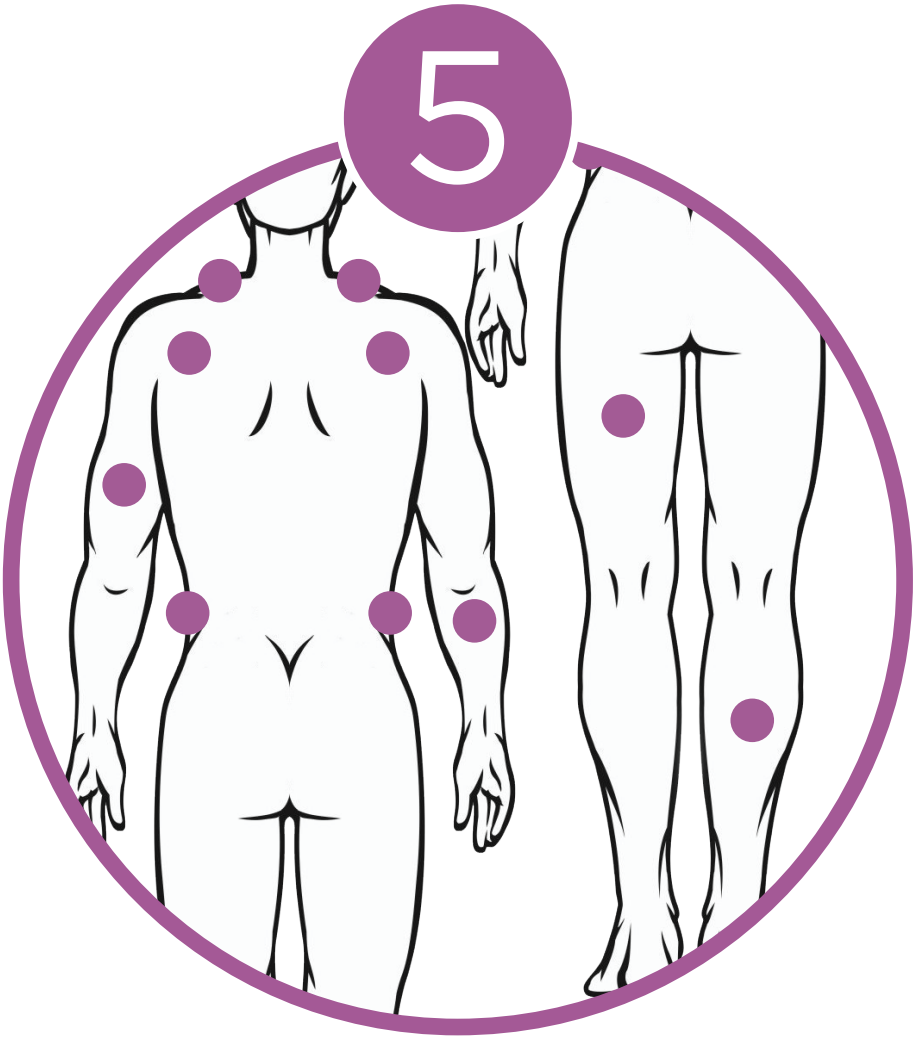

Place the Pain Reliever onto treatment area of choice.

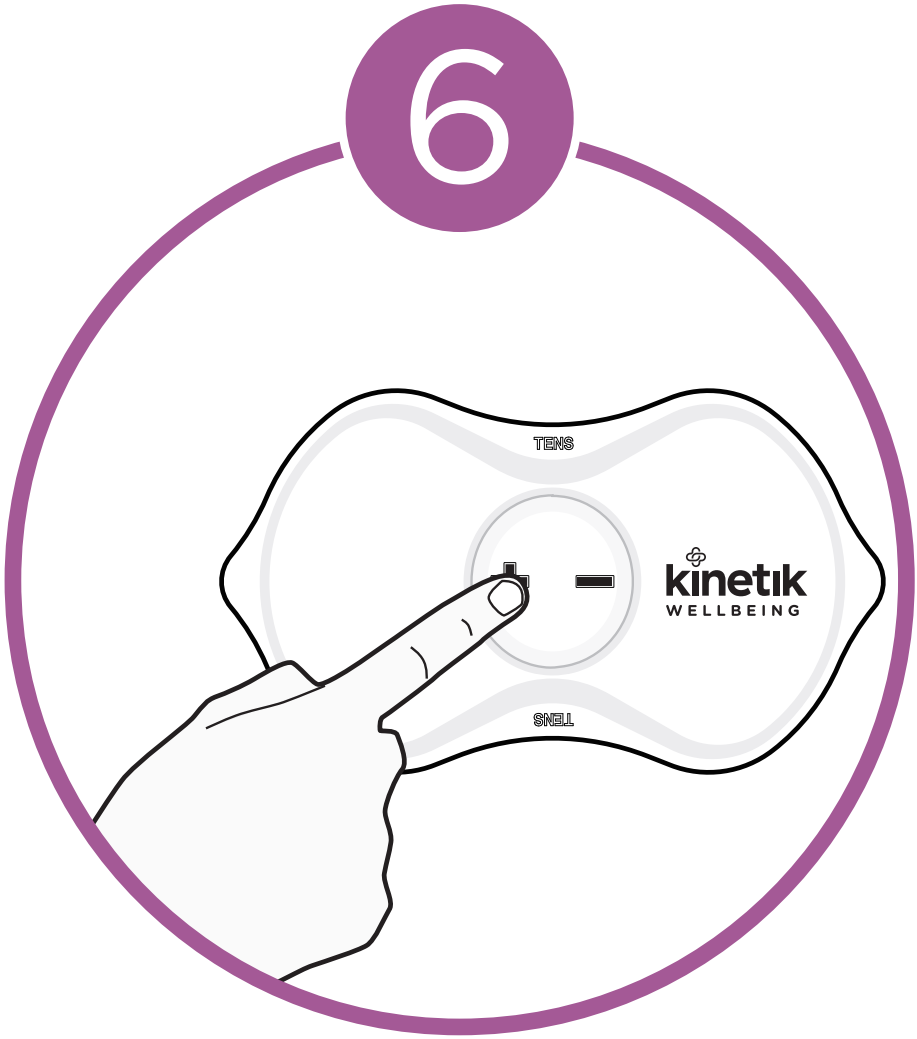

Press + button for
3 seconds to turn on.

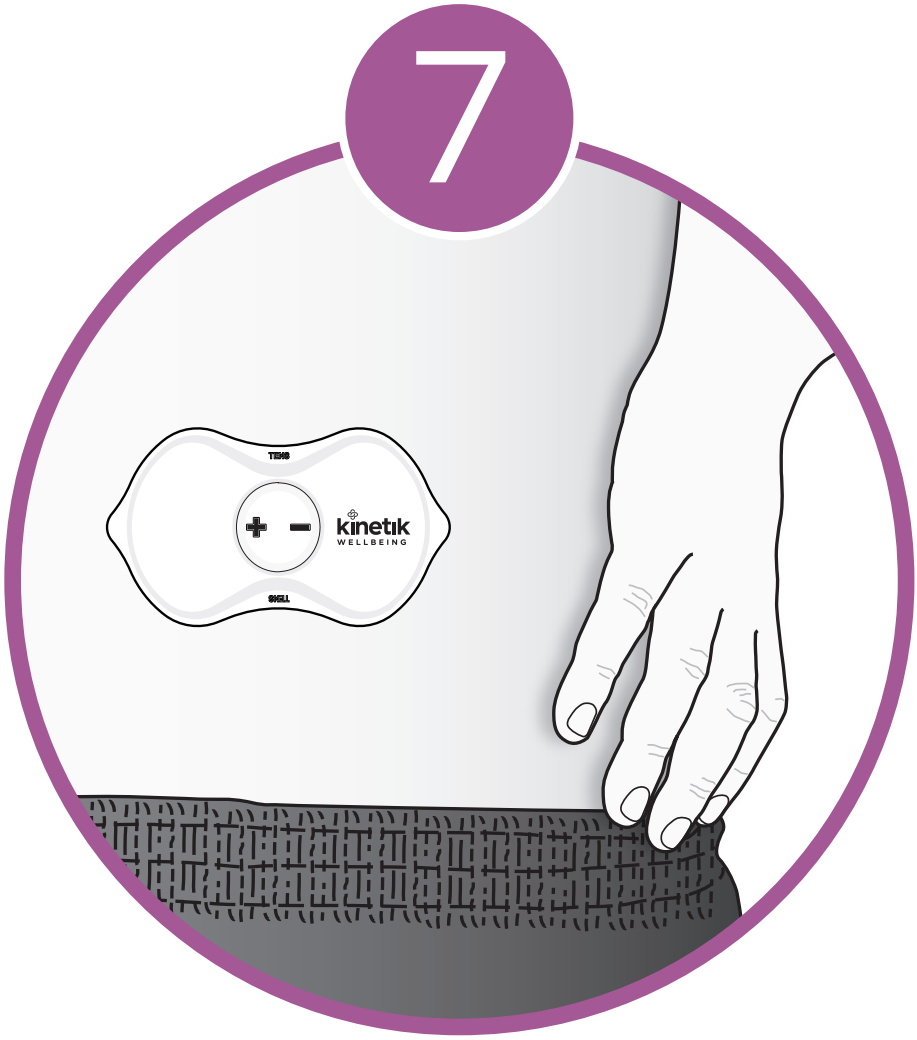

Press the + or − to select desired intensity. Treatment will then take place.

kinetik
WELLBEING

for more information visit :
kinetikwellbeing.com